


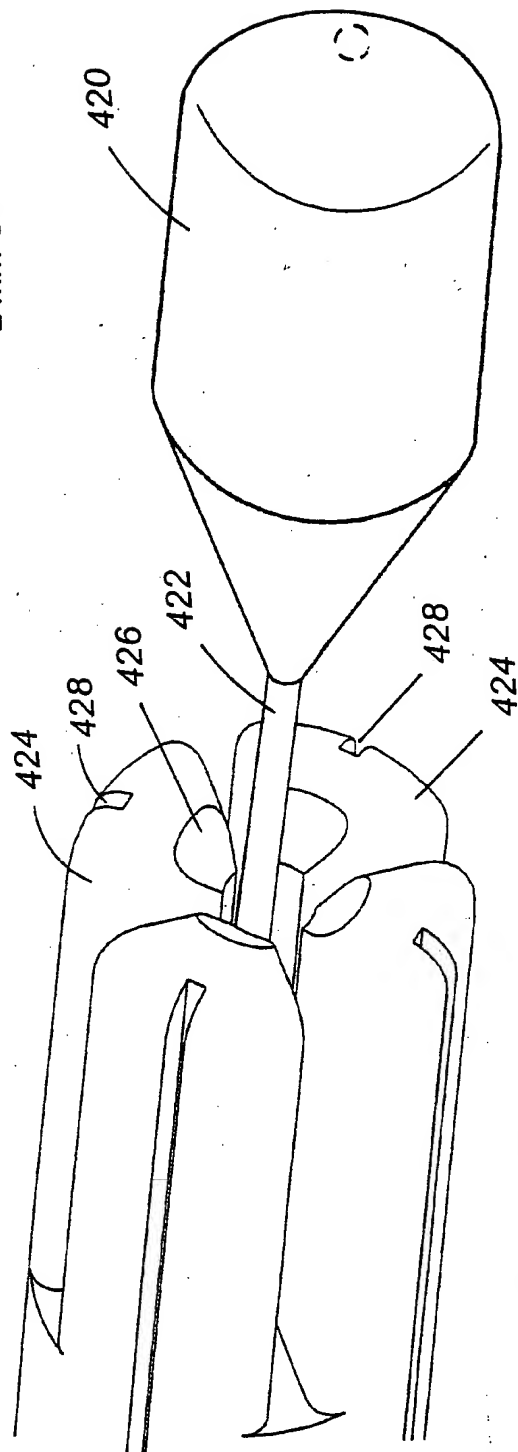


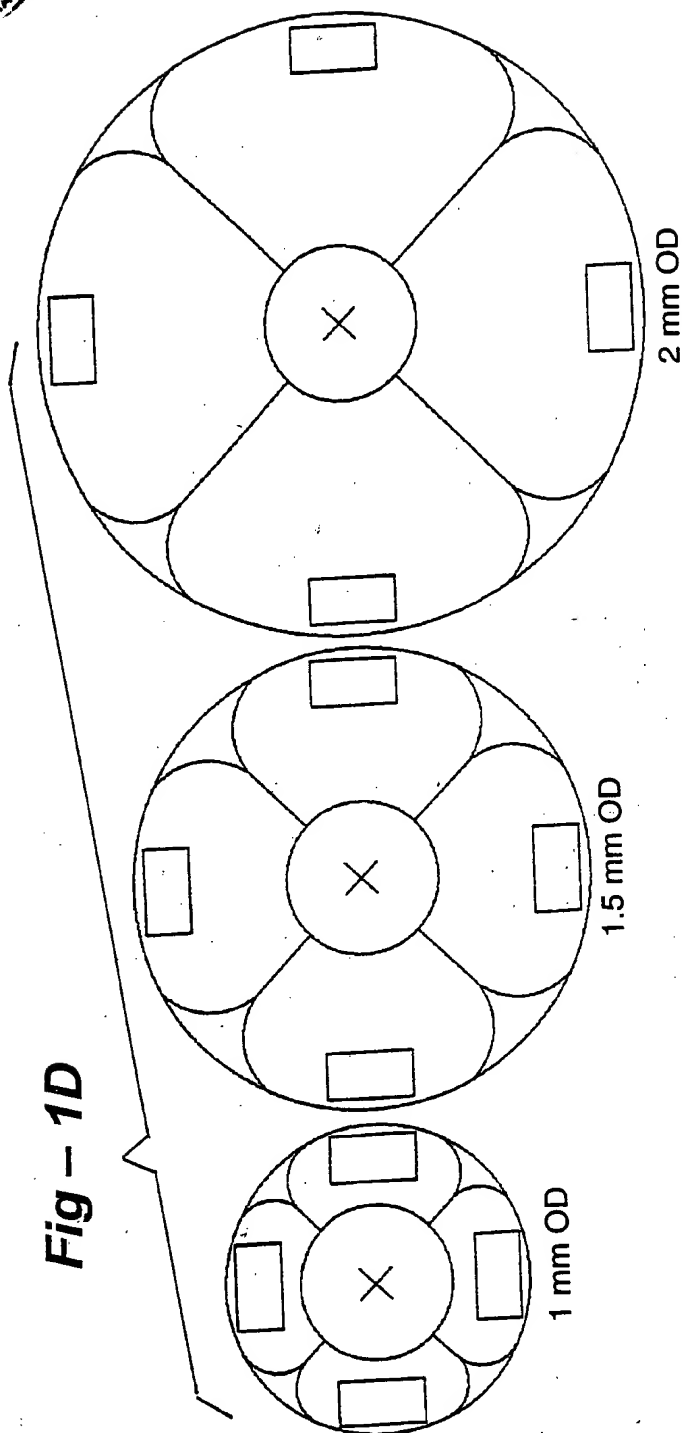


**Fig - 1D**

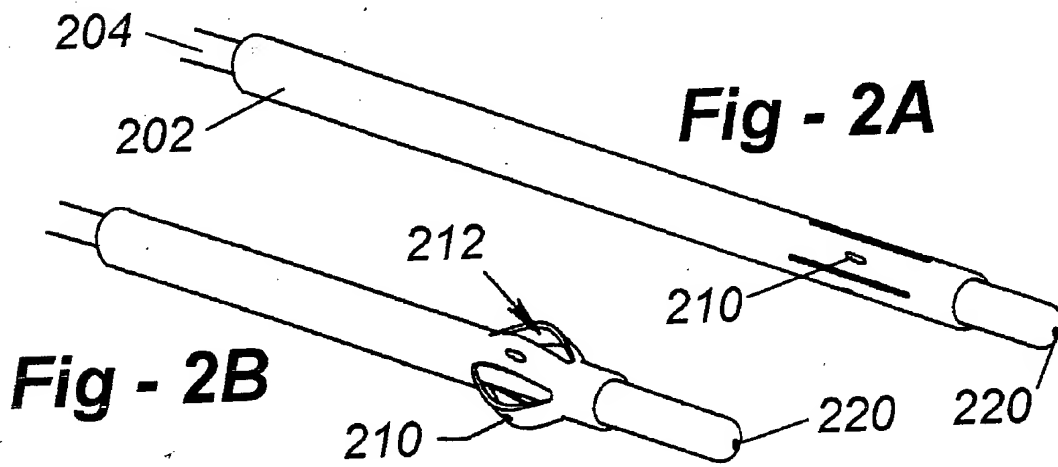


**Fig - 4C**

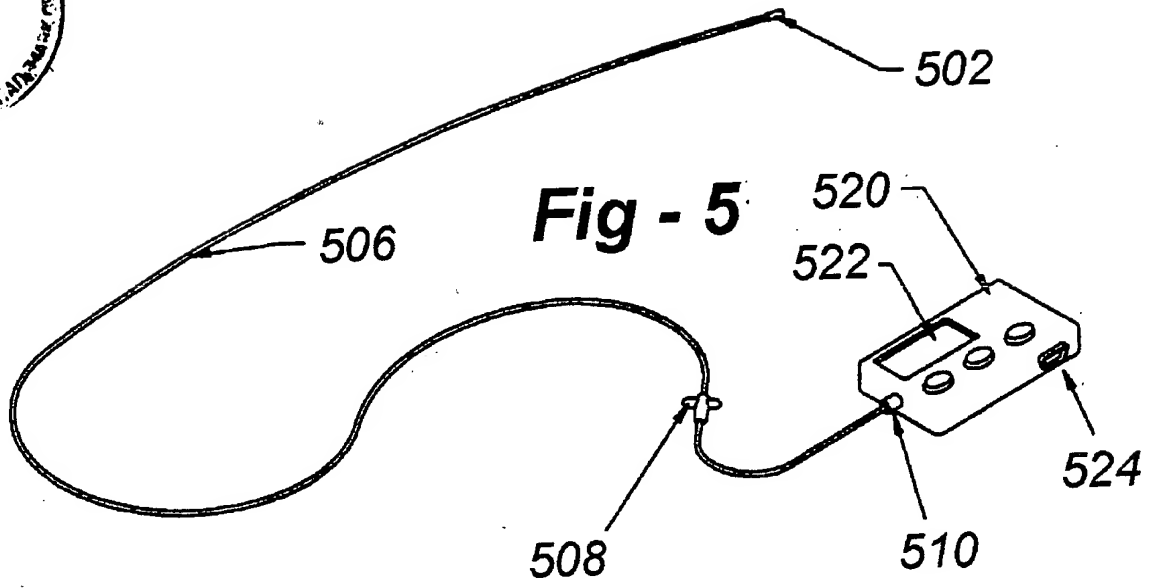


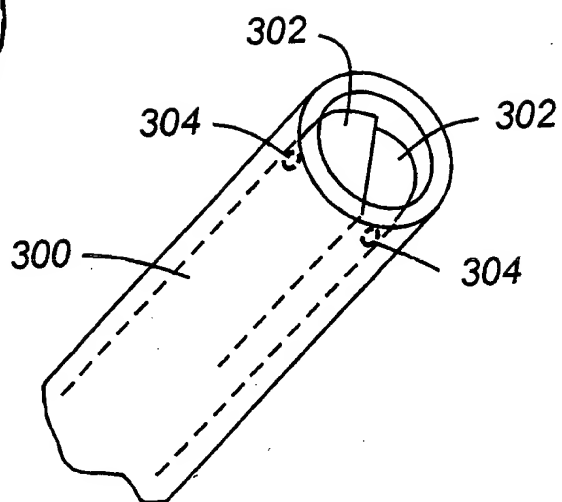

**Fig - 3A**

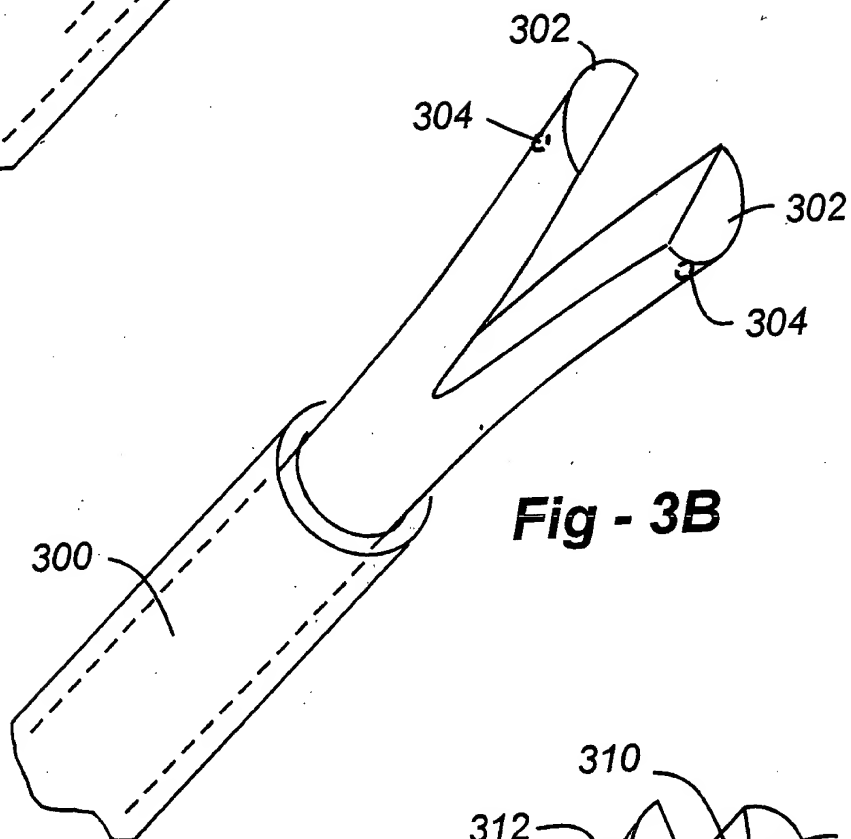


**Fig - 3B**

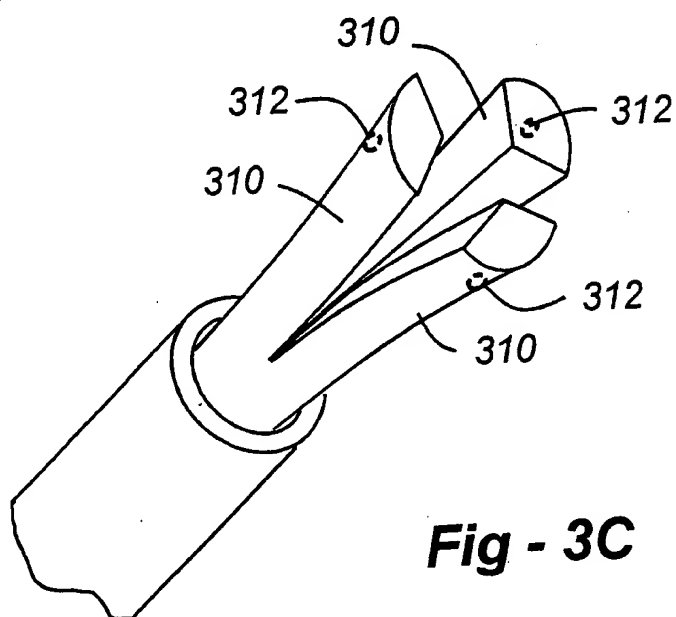



**Fig - 3C**




**Fig - 4A**

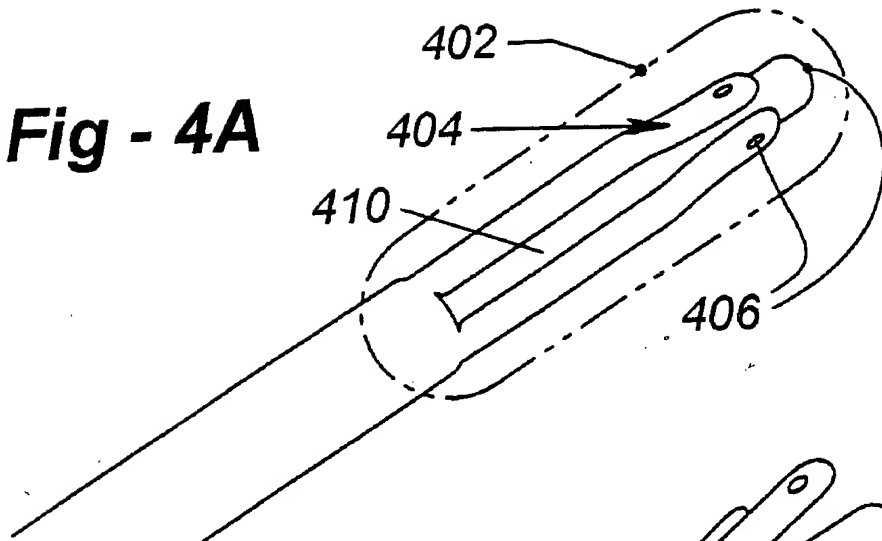


**Fig - 4B**

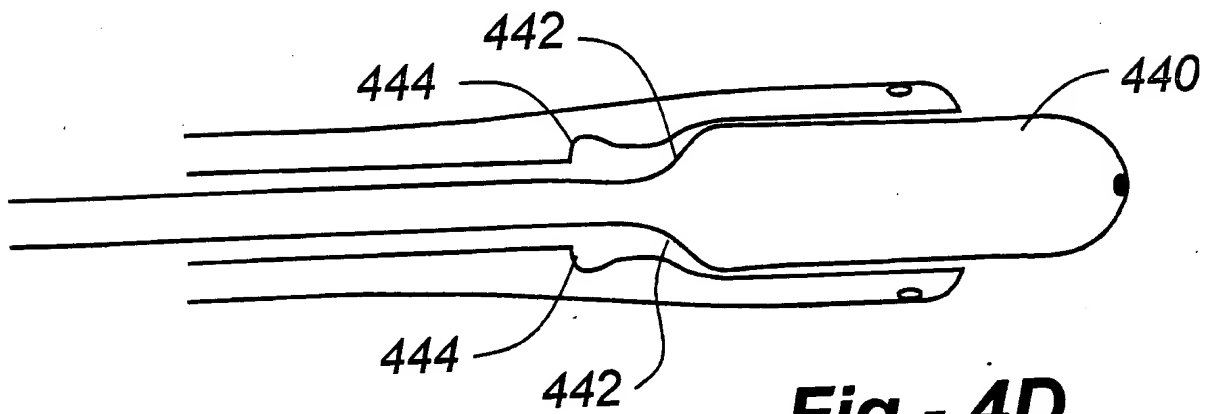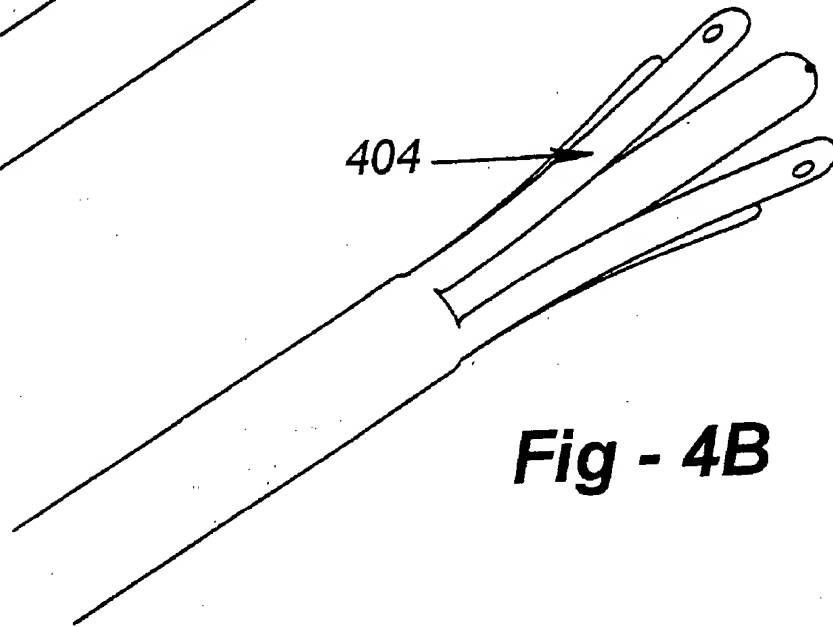

**Fig - 4D**



Absolute & Percent Error for 1, 1.5, 2 mm Diameter Thermal Sensing Catheter

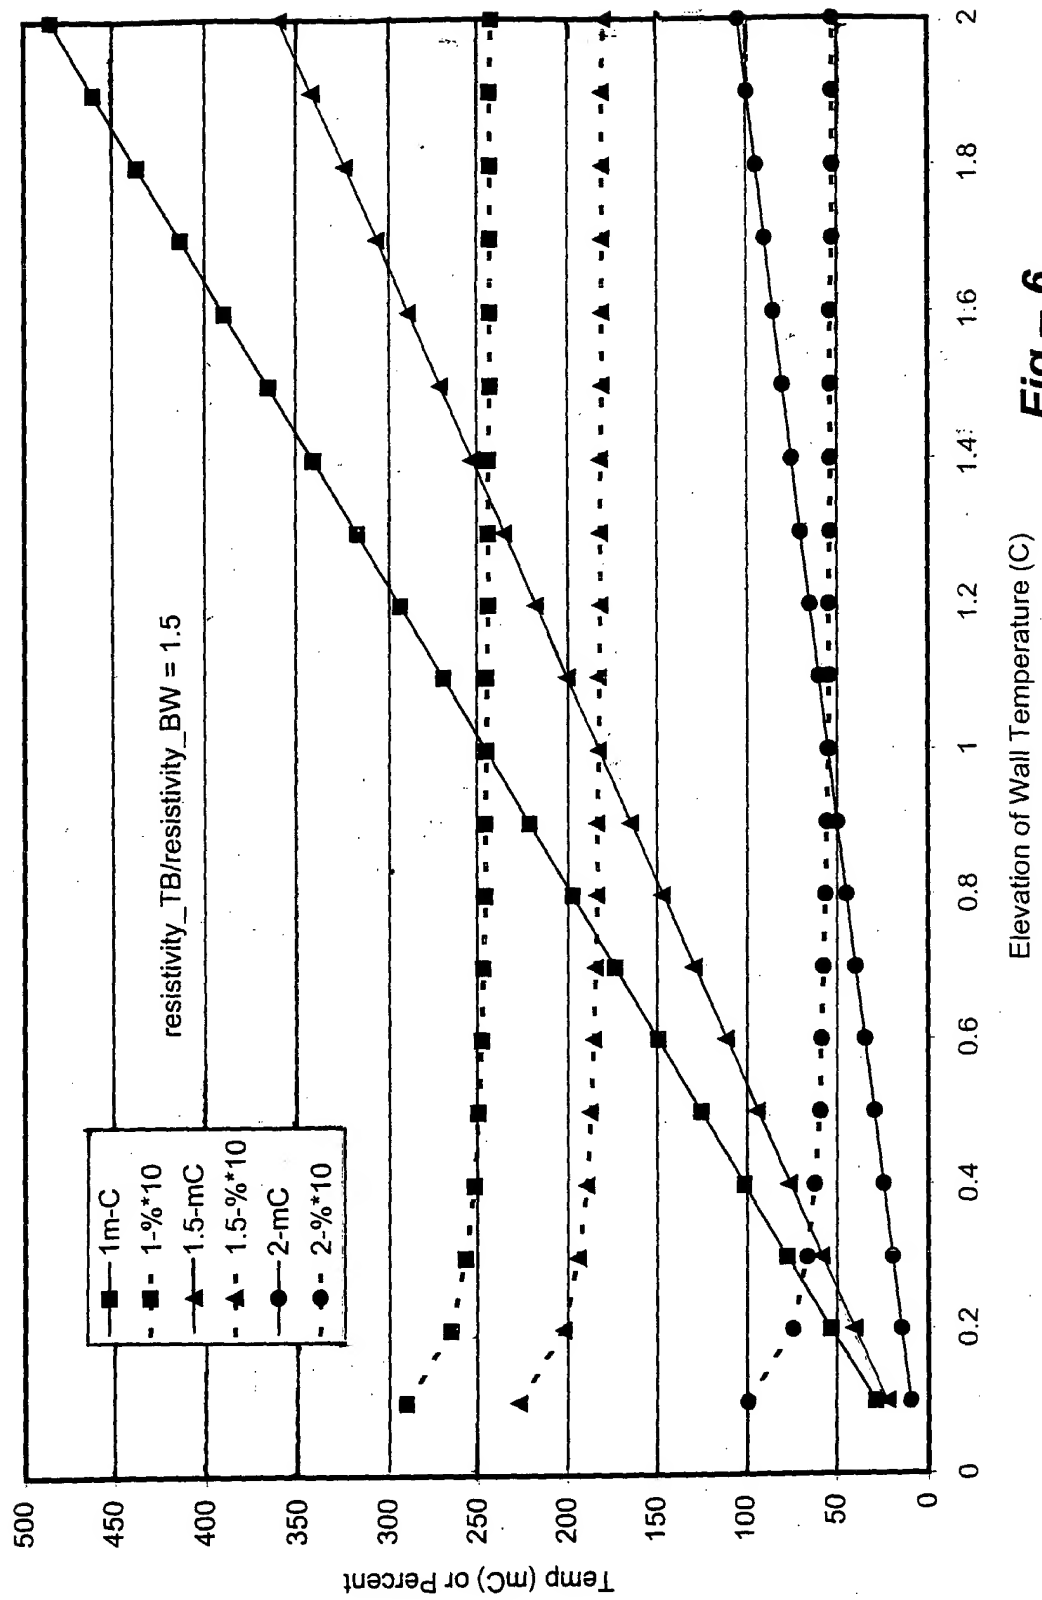



### Third Sensing Arm Assymetry Experiment

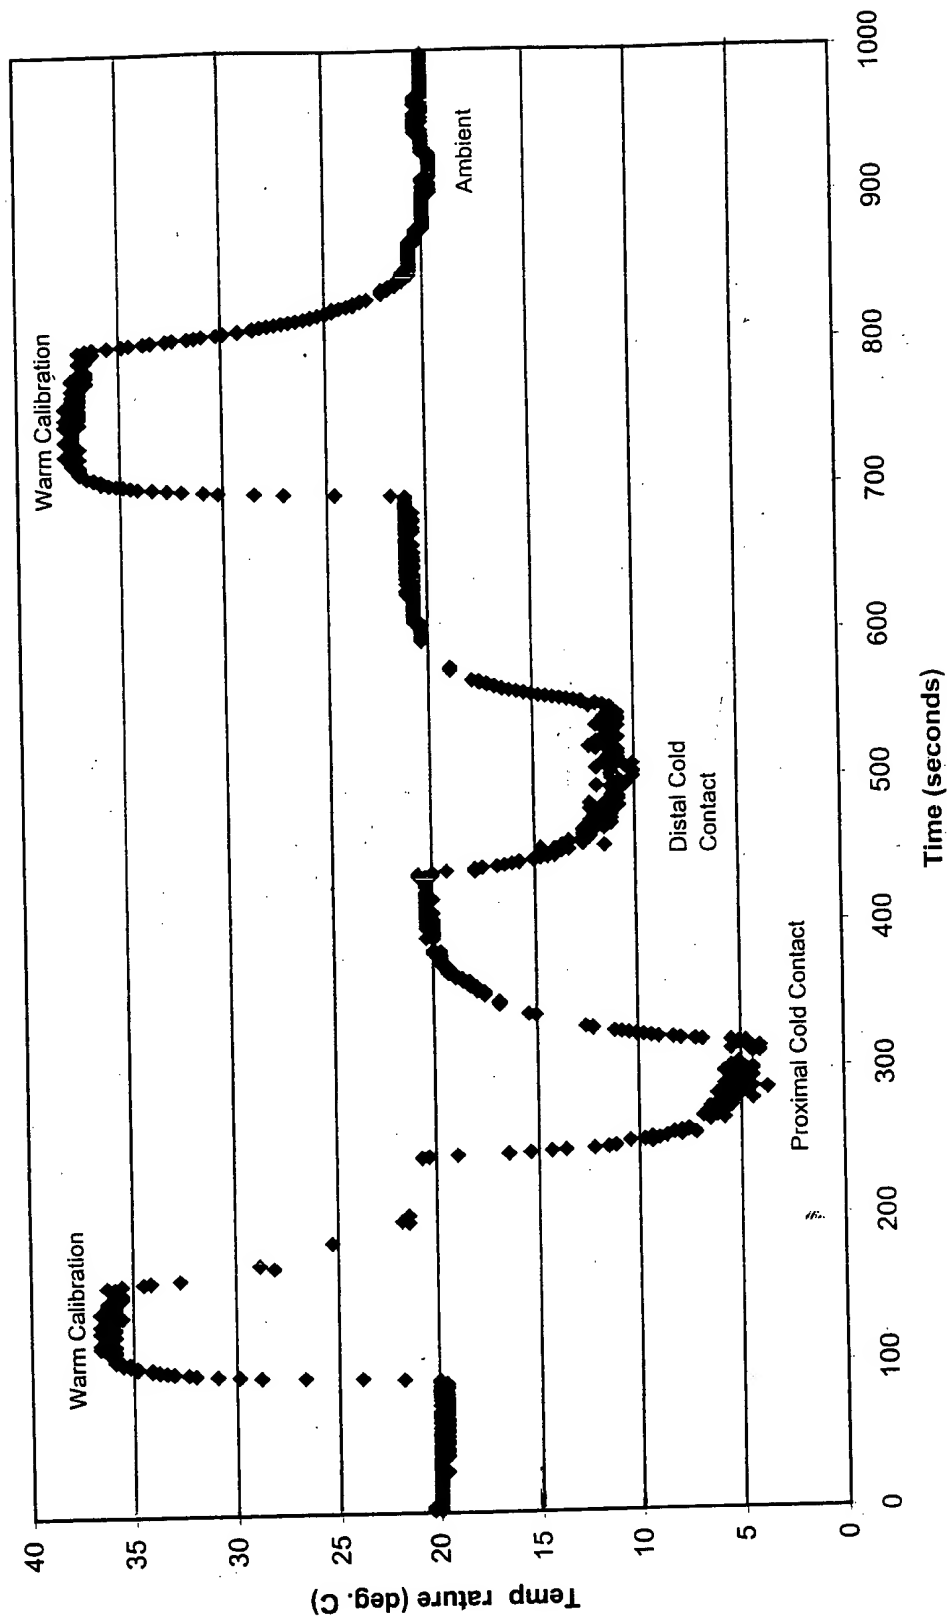


Fig - 7